
TENSATOR®

Changing your Tensabarrier® cassette

Instruction guide

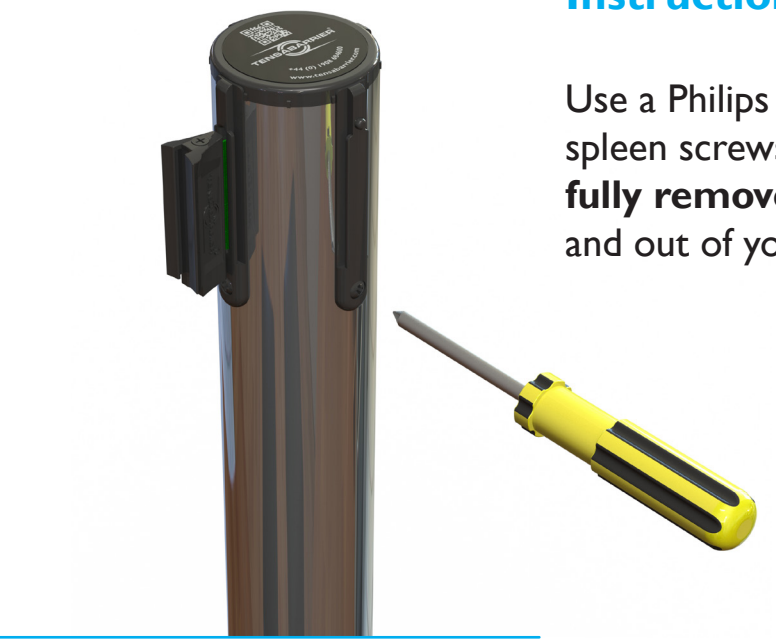

Instructions to remove

Use a Philips head screwdriver to loosen all 4 spleen screws. **It is important that you do not fully remove the screws.** Pull the cassette up and out of your Tensabarrier®.



Instructions to replace

Align new cassette splines with slots in your Tensabarrier®, push down the cassette and tighten screws to secure.

MILTON KEYNES +44 1908 684600
NEW YORK +1 631 666 0300
DUBAI +971 4 2997228
PARIS +33 1 43 09 85 00
FRANKFURT +49 69 3003 890-0
WROCLAW +48 71 359 3800

www.tensatorgroup.com

Owing to the dynamic nature of our business, specifications are constantly being changed and therefore this literature is for informational purposes only. For the most up to date information, please visit our website www.tensatorgroup.com. Tensator makes no warranties, express or implied, in this document. E&OE.